

Tementop

**LKC-1000 Series
Air Quality Monitor
User Manual**

Factory Affecting Air Quality



PM2.5 (Particulate Matter 2.5) refers to fine particles with diameter of 2.5 micrometers or less. Due to its tiny size, PM2.5 can be absorbed into bloodstream and the lungs, so that long-term exposure to high concentration of PM2.5 environment may cause eye and nose irritation, cough, asthma, emphysema, lung disease, heart attacks, cancer and etc.



PM10 (Particulate Matter 10) refers to particulates with a diameter of 10 micrometers or less. Due to the larger size, it's inhalable but penetrates no further than bronchi as larger particles can be filtered out by cilia and mucus of nose and throat. It usually considered as less harmful to health than PM2.5.



HCHO (Formaldehyde) is a colorless and strong-smelling chemical with formula CH_2O or $\text{H}-\text{CHO}$, which has been classified by IARC as Group 1 carcinogen due to its significant dangers to human health. Long-term exposure to just low doses could cause chronic respiratory diseases, nasopharyngeal cancer, colon cancer, brain tumors, nuclear gene mutations and etc.



TVOC (Total Volatile Organic Compounds) refers to various common VOCs including benzene, toluene, styrene, formaldehyde and etc. Due to their volatility as well as toxicity, irritability and carcinogenicity, long-term exposure to TVOCs can cause damage to the skin, liver, kidneys, central nervous system and etc.



Temperature & Humidity may often be ignored however they do have a significant impact on individual's well-being, comfort, health and safety as well as your property. High humidity may lead to an increase in

household air pollutants especially the biological contaminants such as molds, bacteria, viruses and dust mites; cold, low humidity may cause nosebleeds, skin and respiratory irritations, dyspnea, static electricity and etc.




AQI (Air Quality Index) is a quick guide on air quality levels. It aims to indicate how clean or polluted the air is in a way that's easy to understand. It ranges from 0 to 500 that higher values indicate higher air pollution levels and more adverse for health. AQI assessment can be indicated for PM_{2.5}, PM₁₀, O₃, SO₂, NO₂, CO etc. Temtop follows EPA Standards to calculate and focus only for AQI of PM_{2.5} & 10.

Important!

- ★ It is usual for the detector to show higher values when first switched on or not used for an extended period. Please place it in a ventilated area and turn it on for around 30 minutes before testing.
- ★ Do not put the detector in an environment with formaldehyde (HCHO) concentration above 1.0mg/m³ or PM concentration above 500ug/m³ for a long time. Otherwise, the sensor may be damaged and cannot run normally.
- ★ Do not come into contact with organic solvents, which include silica gel and other adhesives, paintings, drugs, oil and high-concentration gases.
- ★ Do not use the detector in a humid environment to maintain detection accuracy.
- ★ Do not cover the air inlet / outlet when using the detector.
- ★ Be cautious of cross interference by ethanol, benzene, ammonia, etc.

Overview

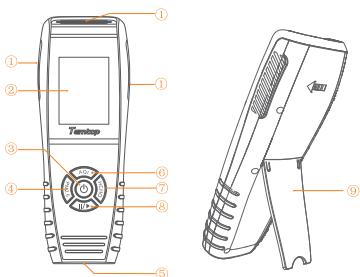

- ① Air Inlet/Outlet ② LCD Screen ③ Power Button
 ④ PM2.5/PM10/Particles Button ⑤ USB Port
 ⑥ AQI/TEMP/HUM/Up Button ⑦ HCHO/TVOC Button
 ⑧ Running/Hold/Setting/Down Button ⑨ Bracket

Function

Model Function	LKC-1000S+ 2nd	LKC-1000S 2nd	LKC-1000S+	LKC-1000S
PM2.5	√	√	√	√
PM10	√	√	√	√
HCHO	√	√	√	√
Particle Count	√	√	√	√
AQI	√	√	√	√
TVOC	√		√	
TEMP&HUM	√	√	√	√
Histogram	√		√	
Data Export	√	√		

Specifications

Model	LKC-1000 Series
Dimensions	177*65.5*32mm (6.9*2.6*1.2 in)
Battery Capacity	3000mAh
Battery Life	15-18h @ Backlight Level 2
Charging Output	DC5V, 1A
Display	TFT color LCD screen
Weight	About 219g (0.48lb)
Operating Environment	Temperature: 0~50°C (32~122°F) Humidity: 0~90%RH
PM2.5	Measuring range: 0-999ug/m ³ Resolution: 0.1ug/m ³ Accuracy: ±10µg/m ³ (0-100µg/m ³) ±10%(100-500µg/m ³)
PM10	Measuring range: 0-999ug/m ³ Resolution: 0.1ug/m ³ Accuracy: ±15µg/m ³ (0-100µg/m ³) ±15%(100-500µg/m ³)
HCHO	Measuring range: 0-2mg/m ³ Resolution: 0.01mg/m ³
TVOC*	Measuring range: 0-5mg/m ³ Resolution: 0.01mg/m ³

*For LKC-1000S+ /LKC-1000S+2nd Only

Note: The above data are from Temtop Laboratory.


Operation

Warning!

- ★ Indoor use: Keep the room/area airtight for 10 minutes to obtain more accurate results.
- ★ If battery level shows , please charge the detector promptly to avoid effects during use (also chargeable when turned off).

1.Switch On/Off



Press and hold  button for 2 seconds to turn on/off the detector.
After initialization, the instrument enters the default interface.

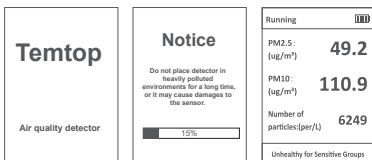


2.Detection

2.1 PM2.5 Button


Please click the  button to view the following four interfaces.

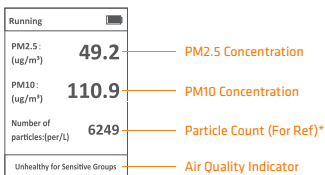

* The particle counts are for reference only. For accurate particle counts please choose a professional particle counter from Temtop.




PM10 Graph View



Particle Graph View

2.2 AQI Button


Please click the  button to view the following four interfaces.
Press and hold  button for 2 seconds to switch between $^{\circ}\text{C}$ or $^{\circ}\text{F}$.




AQI

Temperature


Humidity



AQI Graph View



TEMP Graph View



HUM Graph View

2.3 HCHO Button


Please click the  button to view the following three interfaces.




HCHO Concentration

TVOC Concentration
(LKC-1000S+/1000S+ 2nd)

Humidity



HCHO Graph View



TVOC Graph View
(LKC-1000S+/1000S+ 2nd)

Note:

1) Please click "II/▶" button to switch between running mode and holding mode.

In running mode, the detector always displays currently detected data. In holding mode, the detector paused the detection function and will stop updating data on the screen.

2) Data updates every 3 seconds when x axis value is within 72 seconds. Data updates every 1 minute when x axis value is within 24 minutes. Data updates every 5 minutes when x axis value is within 120 minutes. Data updates every 30 minutes when x axis value is within 12 hours.


3.Settings Menu

Buttons




Button	Setting Function
	Up/Increase
	Down/decrease
	Left
	Right
	Confirm

Press and hold the button for 2 seconds in the main display of "PM2.5, AQI, HCHO" to enter the system settings.



For LKC-1000S / LKC-1000S+ Only



For LKC-1000S 2nd/LKC-1000S+2nd Only


3.1 Power Saving (Example Of Button Operation):

Press the or button to scroll up or down and press the button to confirm.

Press the or button to switch to the item you want to set.

Press the or button to increase or decrease the current value.

Then press the or button to switch to save or exit, and press button to save the setting or exit the interface.

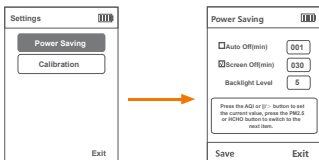


Note: 1. " ☐Auto Off(min) " : Auto power off function is not switched on.

2. " ☒Screen Off(min) " : The screen will automatically switch off after 30 minutes.

3. The "Backlight Level" are divided into 0, 1, 2, 3, 4 and 5.


3.2 Calibration

In this interface, you will you can see figure below.



3.2.1 HCHO Calibration

Press the or button to switch to the "Calibration zero" and press button to calibrate.

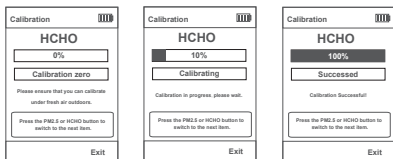

Note:

1. Please ensure that you can calibrate under fresh air outdoors.
2. During the calibration process, please do not perform other operations until the calibration is successful and you return to the previous level screen.

3.2.2 TEMP & HUM Calibration

You can calibrate the temperature and humidity by modifying the "OFF" value.

Formula :

$\text{OFF(TEMP target value)} = \text{TEMP(target value)} - \text{TEMP(current value)} + \text{OFF(TEMP current value)}$.

$\text{OFF(HUM target value)} = \text{HUM(target value)} - \text{HUM(current value)} + \text{OFF(HUM current value)}$.

Example :

If TEMP target value is 25.0, current value is 23.0, current value of OFF(TEMP) is -0.2. Then "OFF(TEMP target value)=25.0-23.0+(-0.2)=+1.8".

If HUM target value is 36.0, current value is 33.0, current value of OFF(HUM) is +1.5. Then "OFF(HUM target value)=36.0-33.0+(+1.5)=+4.5".



3.2.3 PM2.5 Calibration


You can calibrate the PM2.5 value by adjusting the "K" factor.

Formula :

$K(\text{target value}) = \text{PM2.5}(\text{target value}) / \text{PM2.5}(\text{current value}) * K(\text{current value})$.

Example :

If PM2.5 target value is 30.0 $\mu\text{g}/\text{m}^3$, current value is 49.2 $\mu\text{g}/\text{m}^3$, current value of K is 1.00. Then "K(target value) = 30.0/49.2 * 1.00 = 0.61".

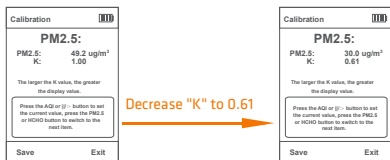

Note: For products calibrated according to ISO standard, K coefficient is 1 by default. It is only recommended that professional engineers perform this adjustment under standard conditions with standard laboratory, or test bin facilities. At the same time, the calibration environment required for P2.5 is relatively high, and the calibration results will be affected by factors such as dust/particle size and different configurations of standard warehouse facilities, etc, so it is strongly recommended that you use this function only under essential conditions or contact us to better support your special needs.

3.3 Date and Time

In this interface, you will see the figure below.

Date and Time

2020-01-01

09:30:00

Press the AQI or [j] > button to set the current value, press the PM2.5 or HCHO button to switch to the next item.

Save Exit

3.4 Storage Interval

In this interface, you will see the figure below.

Storage Interval

Interval(Min) 60

Press the AQI or [j] > button to set the current value, press the PM2.5 or HCHO button to switch to the next item.

Save Exit

Note: The recording intervals are divided into 01, 05, 10, 30, and 60 min.

3.5 Data Export *


In this interface, you will see the following tips.

Export

The instrument is testing whether the USB is connected correctly...

*** For LKC-1000S 2nd /LKC-1000S+ 2nd Only.**

If connected to the computer successfully by the USB cable, the detector will pop up a tip USB connection successful; If not, it will remind you of the failure (See the figures below).



After successful connection, the detector creates a removable storage device "TEMTOP" on the computer, which contains a folder named "HISTORY". This history folder contains a history file named after the time, e.g. "20230601". The history file is in CSV format and lists information such as date, PM2.5, PM10, PARTICLES, AQI, HCHO, TVOC, Temperature, Humidity, etc. (see figure below). Please save it to your computer for viewing.

DATE	PM2.5 ($\mu\text{g}/\text{m}^3$)	PM10 ($\mu\text{g}/\text{m}^3$)	PARTICLES	AQI	HCHO (mg/m^3)	TVOC* (mg/m^3)	TEMP	HUMI (%)	TEMPUNIT
2023/6/1 9:01:40	34.6	56.3	5277	98	0.04	0.17	26	61.4	C
2023/6/1 9:02:40	36.6	61.6	5228	103	0.03	0.14	26	61.4	C
2023/6/1 9:03:40	34.1	56.6	5218	97	0.04	0.16	26	61.4	C
2023/6/1 9:04:40	35	56.8	5288	99	0.04	0.16	26	61.4	C
2023/6/1 9:05:40	35.3	57.7	5341	93	0.04	0.17	26	61.4	C

* For LKC-1000S 2nd /LKC-1000S+ 2nd Only.

After copying and viewing historical data, please press  to exit (see figure below).



Note: USB connected successfully. During the data export process, please do not unplug the USB. If you want to exit the USB connection mode, press the  button!

Air Quality Parameter for Reference

Status Pollutant	Good	Moderate	Unhealthy for Sensitive Groups	Unhealthy	Very Unhealthy	Hazardous
PM2.5 ($\mu\text{g}/\text{m}^3$)	≤ 12	12.1~35.4	35.5~55.4	55.5~150.4	150.5~250.4	≥ 250.5
PM10 ($\mu\text{g}/\text{m}^3$)	≤ 54	55~154	155~254	255~354	355~424	≥ 425
AQI*	≤ 50	51~100	101~150	151~200	201~300	≥ 301

Pollutant \ Status	Healthy	Unhealthy
HCHO (mg/m^3)	≤ 0.1	> 0.1
TVOC (mg/m^3)	≤ 0.5	> 0.5

*Refers to EPA standards, with PM2.5 as the main responsible pollutant.

What's Included

LKC-1000 Series Detector x 1

USB Cable x 1

User Manual x 1

FAQ

Q: Why data reading is unstable?

A: If the airflow in the current sampling space is in an unstable state, such as strong wind, the concentration of particulate matter in the air will be unevenly distributed, and will vary greatly with the surrounding airflow, resulting in large differences in measured values.

Q: Why humidifiers can cause rising particulate matter readings?

A: Our sensors use the principle of light scattering. When using a humidifier, the humidifier will spray many small droplets of water. Excessive humidity and moisture in the air will cause dust particles to absorb water and swell, which will affect the scattering of light and cause deviations in sensor readings.

Q: Why is the data high after booting?

A: The reason why the data is high when you first turn on the sensor is that when the sensor starts to work, the fan will run at full speed, and it will take a while (about 1-2 minutes) for the fan to run stably. At this time, the airflow in the air duct will be stable, and the data will gradually become stable.

Q: AQI/ PM2.5 and other values, why the measured value is inconsistent with the official announcement?

A: The AQI/PM2.5 shown on the display is a measurement

of the space where the device is located. The measured value published on the Internet or official websites is the average value of several monitoring points, and each measurement point will be different. At the same time, according to the regulations of EPA and WHO, the AQI value is calculated based on the highest value among the five pollutants in the atmosphere on that day. In the past ten years, the local AQI in the United States has basically been calculated with the value of PM2.5/10, and sometimes with the value of O₃.

Q: Which the HCHO reading inaccurate or overestimated at some points?

A: As Temtop uses a high-precision electrochemical HCHO sensor, its electrochemical reaction characteristics could also respond to other gases besides formaldehyde. This table lists the most common gases that interfere with relative sensitivities of HCHO sensor.

Interference Gas	Relative Sensitivity (%)
Carbon monoxide(CO)	1
Hydrogen (H ₂)	0.1
Ethyl alcohol	50
Phenols	7
Sulphur dioxide(SO ₂)	12
Ammoniak (NH ₃)	0

Warranty

Temtop warrants the included detector for 1 year from the date of original purchase. The item can be exchanged or returned within 30 days if the defect is not caused by artificial damage.

Item	Warranty Period
Detector	1 year included
Accessories	N/A

Before return or delivery for repair, please check if the following items are ready:

	Detector & Accessories	Complete Package	Proof of Purchase*	Gift (if any)
Return	√	√	√	√
Exchange	√	√	√	
Repair	√		√	

* Including invoice, order number and etc.

Temtop warranty does NOT include:

- Malfunction or damages caused by artificial damage or modification.
- Other deliberate damages.
- Damage caused by natural events.



Elitech Technology, Inc.

2528 Qume Dr, Ste 2
San Jose, CA 95131 USA
Tel: (+1) 408-898-2866
Sales: sales@temtopus.com
Website: www.temtopus.com

Elitech (UK) Limited

Unit 13 Greenwich Business Park,
53 Norman Road, London, SE10 9QF
Tel: (+44)208-858-1888
Support: service@elitech.uk.com
Website: www.temtop.co.uk

Elitech Brazil Ltda

R.Dona Rosalina,90-Lgara, Canoas-RS
92410-695,Brazil
Tel: (+55)51-3939-8634
Sales: brasil@e-elitech.com
Website: www.elitechbrasil.com.br

V1.4

Made in China